




Specimen_001-Buse 100 Standard

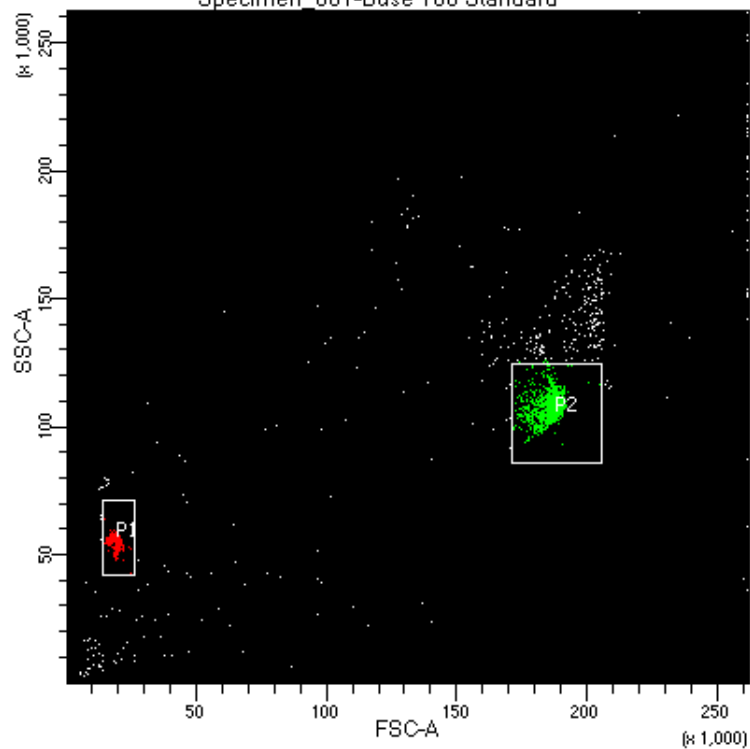


Specimen_001-Buse 100 Standard

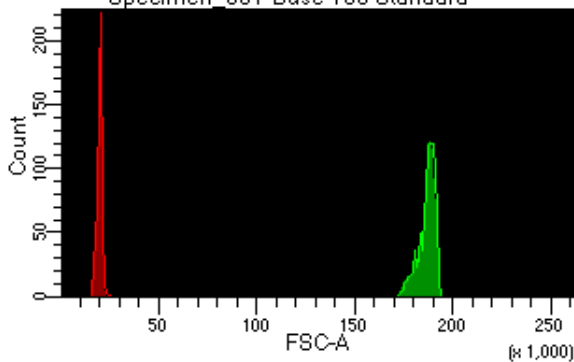


Specimen_001-Buse 100 Standard

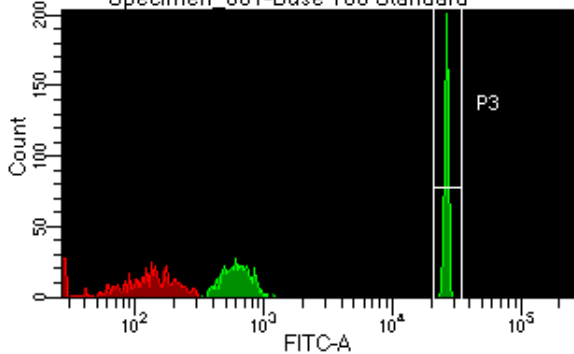

Specimen_001-Buse 100 Standard

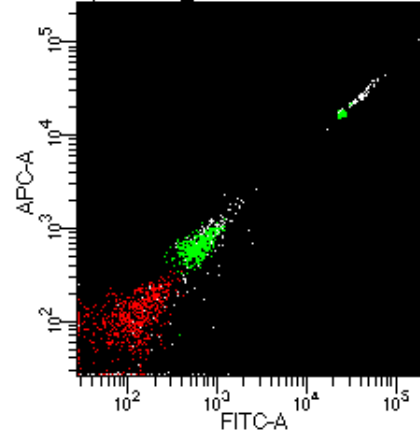

Specimen_001-Buse 100 Standard

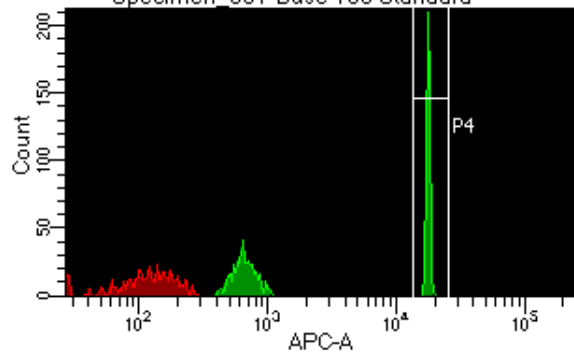

| Tube Name: | Buse 100 Standard | | | | |
|--|------------------------------|---------|---------------|----------------|---------------|
| Record Date: | May 26, 2015 11:53:19 AM | | | | |
| SOP: | Administrator | | | | |
| GUID: | 5a4dc12e-fd31-4294-9c4e-7... | | | | |
| Population | #Events | %Parent | FSC-A %rCV | FITC-A Mean | APC-A Mean |
| <input checked="" type="checkbox"/> P3 | 574 | 28.6 | 2.4 | 25,915 | 17,597 |
| <input checked="" type="checkbox"/> P2 | ##### | ##### | 1.9 | 13,192 | 9,061 |
| <input checked="" type="checkbox"/> P4 | 606 | 30.2 | 2.5 | 26,433 | 17,878 |

