



[Ungated] FS




[FCblue@2.0] FL1




Gate	Number	X-AMean	HP	X-CV
All	10,815	512.65		2.14
FCblue@2.0	5,000	837.06		0.66
FCred	2,734	304.99		0.84
FCviolet	2,295	121.20		2.14

Gate	Number	X-AMean	HP	X-CV
All	5,000	549.17		0.69
FL1@2.0	4,818	550.62		0.69

[FCblue@2.0] FL2

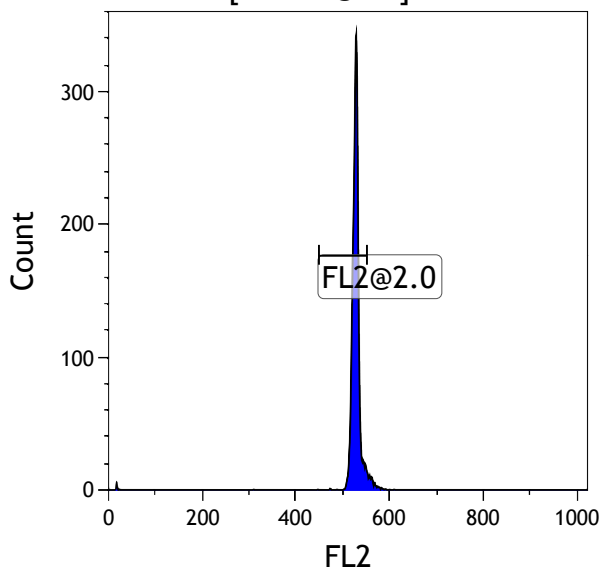

[FCblue@2.0] FL3




Gate	Number	X-AMean	HP	X-CV
All	5,000	527.19		0.96
FL2@2.0	4,770	528.30		0.96

Gate	Number	X-AMean	HP	X-CV
All	5,000	539.36		0.78
FL3@2.0	4,499	539.47		0.78


Gallios FlowCheck 2015-09-07  
Flow-Check Pro - 10 color - Acquisition

[FCblue@2.0] FL4




Gate	Number	X-AMean	HP	X-CV
All	5,000	490.70		0.95
FL4@2.0	4,864	491.79		0.95

[FCblue@2.0] FL5




Gate	Number	X-AMean	HP	X-CV
All	5,000	558.25		1.29
FL5@2.5	726	545.65		0.23

[FCred] FL6




Gate	Number	X-AMean	HP	X-CV
All	2,734	508.05		0.83
FL6@3.0	2,691	514.11		0.83

[FCred] FL7




Gate	Number	X-AMean	HP	X-CV
All	2,734	461.64		1.01
FL7@3.0	2,700	467.30		1.01

[FCred] FL8




Gate	Number	X-AMean	HP	X-CV
All	2,734	519.57		1.06
FL8@3.0	2,622	524.89		1.06

[FCviolet] FL9



Gate	Number	X-AMean	HP	X-CV
All	2,295	490.93		1.02
FL9@4.0	2,265	497.08		1.02

[FCviolet] FL10



Gate	Number	X-AMean	HP	X-CV
All	2,295	514.33		1.06
FL10@4.0	2,273	519.29		1.06